


EasyCal Calibration Software

The comprehensive solution to calibration work and management



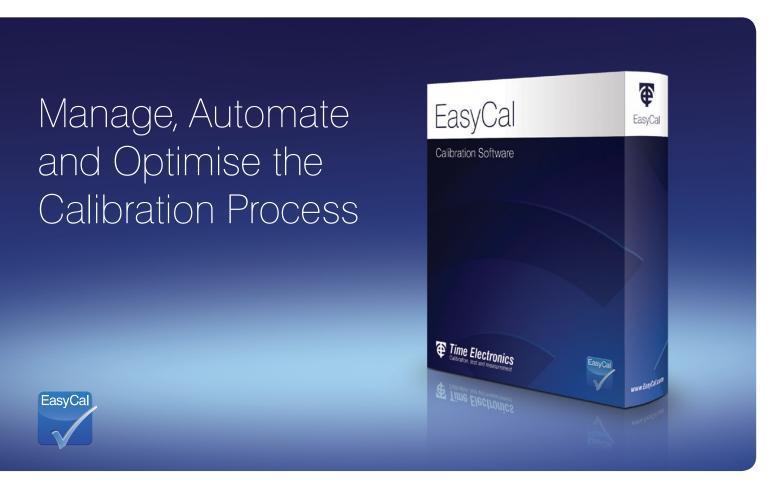

About Easycal

EasyCal is a complete software package with features covering all aspects of calibration work and management. It is designed to reduce workload, improve efficiency, and provide the essential platform for companies looking to create and sustain an effective calibration program. The comprehensive features simplify the administration process from reminder reports through to despatch. With a familiar and intuitive user interface all operators can quickly learn and navigate through the applications. This allows fast, straightforward implementation and integration of the software.

Communication and Control

EasyCal automates calibration runs by allowing the user to remotely control and communicate with compatible calibrators and DMMs. User friendly features and controls aid the process to further decrease calibration times. EasyCal can also read back values and data from compatible Time Electronics pressure and process instruments, and can be used with external instruments such as dry block calibrators.

For Multiple Industries and Disciplines

EasyCal is a versatile solution to multi-device calibration with the comprehensive functionality that is required across industries. It is globally used as the principal software in both calibration businesses and companies with on-site test facilities.


EasyCal is also designed for universal testing applications and can cover a wide range of disciplines. Users can calibrate and verify various instruments and devices: electrical and electronic; level, pressure, and flow; temperature and loop; mechanical and dimensional.

Features

- Communicate with calibrators, DMMs, bench modules
- Automated planning and scheduling
- · For use with multiple devices and instruments
- Print/email/store certificates and reports
- Network compatible
- Produce calibration labels
- · Quickly generate procedures using templates
- 1200+ pre-written test procedures included
- · Calibration due reminder system
- E-mail reminder letters and lists
- · Customise reports and certificates
- Create PDF reports and certificates (PDF engine)
- Print and read bar codes
- Universal instrument control
- HART and Foundation Fieldbus communication
- Secure user log in and electronic signatures
- Create uncertainty tables for laboratory & site
- · WebCert feature for online certificates



Automating the Calibration Process with EasyCal

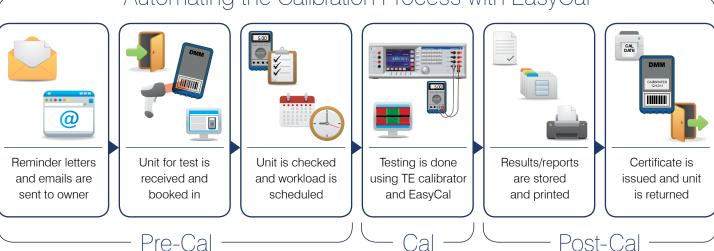

EasyCal: For the Calibration Process

Automating the calibration process brings important benefits and provides increased speed of calibration and consistency of results.

Pre-Calibration: The calibration management features of EasyCal make the planning and organisation of instrumentation calibration simple. A recall/reminder system informs the user of upcoming jobs, and search functions allow the user to quickly identify a unit for test.

Calibration: EasyCal controlled calibration significantly decreases testing times, meaning less instrument downtime and faster turnaround. This improves throughput meaning greater return on investment. EasyCal optimises the process by allowing the user to create procedures quickly and easily with the help of the included design wizards and pre-written templates.

Post Calibration: Easily produce calibration certificates and reports to ISO 9001, ISO 17025, and other quality standards. These can be printed, stored, or emailed as PDFs. EasyCal has a selection of preformatted certificate templates suitable for displaying typical calibration results.



The Core Benefits of using EasyCal


Achieve compliance with quality standards


- Automated document control ensures conformity and quality
- Establish procedures to maintain repeatability and monitor quality
- · Schedule and maintain calibration intervals.
- Evidence of traceability to national standards
- · Record calibration environmental conditions
- · Produce calibration labels, maintain calibration history
- Reduce possibilities for errors or omissions
- Electronic record retention ensures integrity for successful audits


Create an efficient control and management system

- · Reduce testing times
- · Eliminate continual outsourcing calibration costs
- · Full control over the calibration process
- Improve turnaround
- Quick and easy solution to instrument analysis when needed
- · Internal scheduling for calibrations. No external factors
- Centralised document management
- On demand networked review of certificates and reports



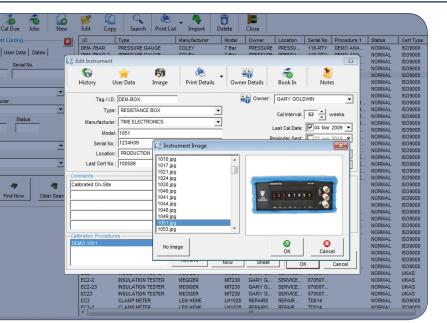

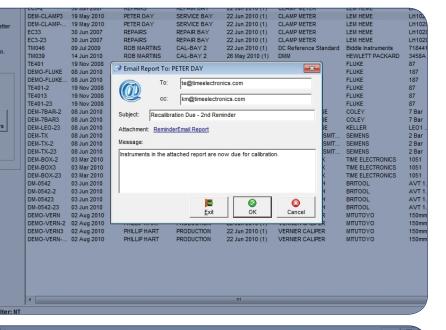

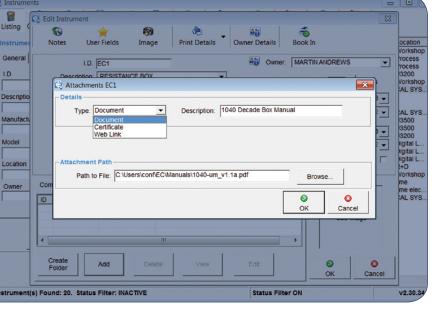

Inventory, Reminders, and Jobs

A comprehensive inventory database can be created and customised to company requirements. For internal calibration and quality management, departments and users can be specified. Alternatively EasyCal can be used as the controlling system for a calibration business based around customers and owners.

Search

A powerful search feature enables the user to enter specific criteria to quickly find the required data. When adding details the user is aided by drop-down lists, which automatically update when new information is added.

Input Fields

Used to add details such as ID and serial number. manufacturer and model, instrument status and service notes. In addition custom fields can be created to integrate with a company system. Images can be uploaded to provide further reference.

Instrument Recall and Reminder System

Instruments which are due for calibration are listed on screen. Reminder letters and lists can be printed or emailed directly to the customer or department. An advanced notice period can be set to bring forward the recall date allowing for response time.

Job Management

When a unit for test is booked in the job process starts. Specific information about the job is entered; such as 'service required', 'sub contracted' and 'accessories supplied'. A job sheet and label can be produced at this stage to accompany the instrument. As the job is put through the system these parameters can be updated, for example 'quote price', 'job status' and 'invoiced'.

Attachments

Create links to technical files, specifications, web pages, word documents, videos, and more. These can be set to automatically display prior to the calibration run.

Devices and Standards used for Calibration

Traceability information for instruments and standards that perform the calibration work is stored and maintained by EasyCal.

Uncertainties

Uncertainty tables for laboratory and site can be created for each calibrating instrument. These are then automatically processed and applied to certificates as required.



Procedure Writing and Editing

Creating and editing test procedures is made simple with an intuitive, user-friendly interface. Editing test information can be done by adding, inserting, or copy and pasting. EasyCal keeps track of each time a procedure is edited.

Procedure Library

A calibration library comprising of over 1200 procedures covering a wide variety of instruments and devices is included as standard.

Procedure Templates

Procedure templates for multimeters, clamp meters, decade boxes, insulation testers, and more can be used for creating any new procedures as required.

Fast Procedure Creation and Editing

Copy and paste multiple tests. Globally edit a group of tests. Colour coded listing helps sort and identify different test types.

Procedure Simulation

The Calibration Run Simulator enables a procedure to be tested without the need for a controlling instrument. To further assist with development of procedures a test can also be edited during the actual calibration run.

Format Certificates


Colour code and add borders to test group titles. Add column headers where a change of layout is required. A preview feature allows the user to check the certificate layout to determine if formatting is correct.


Conversion Tables


Conversion tables for thermocouples, RTDs, current transformers, and clamp meter adaptors are included. Alternatively user-defined tables can be created.

Remote Commands


For more complex instrument control, commands can be sent on a test-by-test basis or run as a script. Closed loop calibration is also achievable using the universal readback feature. This allows EasyCal to control third party calibration equipment and communicate with devices under test.

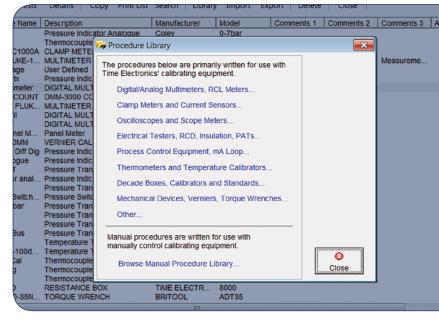


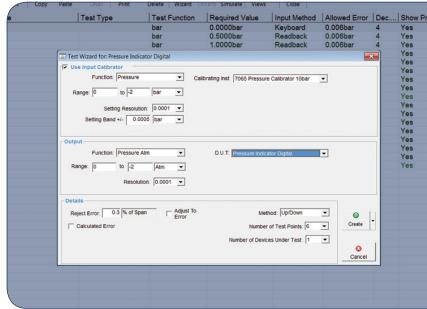


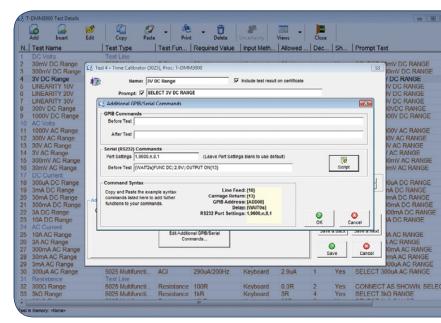

Overview of applications and features

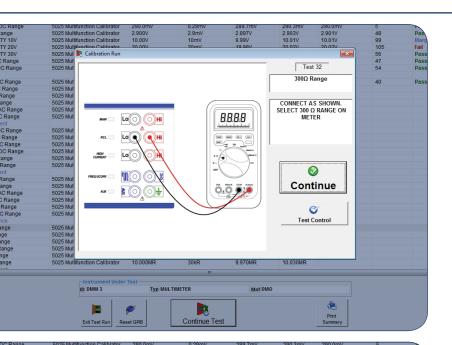

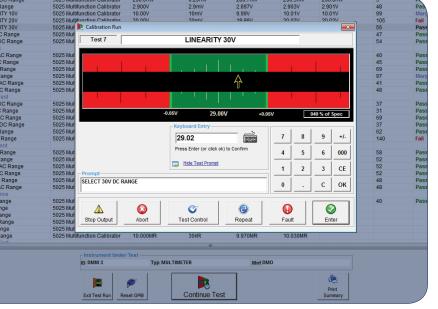

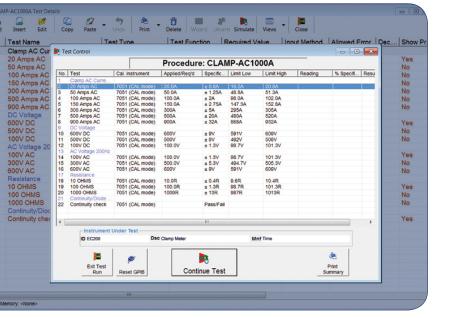

Instrument and Device Calibration

Automated calibration run provides fast and accurate collection of data, whether using direct instrument control or manual entry. EasyCal guides the operator through the procedure using graphical test screens and user prompts.

Search

Selection of the device under test is quick and easy. With the use of a barcode scanner this selection becomes automatic.

Calibration Prompts

Text and graphical prompts aid the user with instrument range selection and connection. So even the most complex calibrations can be performed with relative ease.

Graphical Test Screen

The calibration run is made simple and efficient by a graphical user-interface, which increases speed of data entry. The colour coded indication bar displays the test limits. This allows the operator to easily identify out of tolerance results.

Test Control

At any stage during the calibration run a summary can be displayed, this includes both completed and remaining tests. Colour coding indicates tests passed or failed. The operator is able to move forward or backward through the procedure as required.

End of Calibration Run

Data for every test is stored, including a snap shot of the procedure used. If required calibration comments and service history can be updated. The operator is able to print the certificate, produce a calibration label and/or store the results to be issued as required.

Recovery Mode

If for any reason a calibration run is interrupted, recovery mode allows the user resume from the point of termination.

Calibration Test Forms

Alternatively 'calibration test forms' for hand written results are available. This data is then entered manually into EasyCal at a later date.



Certificates/Reports/Data Management

Produce, print, and store calibration certificates, reports, and labels. Simple search facilities enable the user to locate any data on demand. Keeping track of instrument history and servicing is made easy.

Certificate Templates

A range of pre-formatted templates are available for immediate use. A company logo can be added without the need for 3rd party software.

Electronic Signatures

Password protected electronic signatures allow management to approve certificates. In addition a scanned image of the signature can automatically be inserted, eliminating the need to print certificates.

Built-in PDF Engine

Generate PDF reports and certificates ready for emailing and universal review.

Calibration Reports

Documented traceability provides a recorded audit trail. Reports showing calibration duration times can assist with costing and assessments.

Archive


The results database can be streamlined by using the archive feature. This improves data organisation and management. Archives are quickly retrieved, giving instant access to historical certificate data.


Import and Export


Exchange data from one system to another using the import/export feature. This method is ideal for site and field calibration work, where data is recorded externally then uploaded to the main database upon return.

Customise

Crystal Reports (optional) allows full modification of certificate, label, and report layouts. Design custom reports using queries, formulas, and running totals.

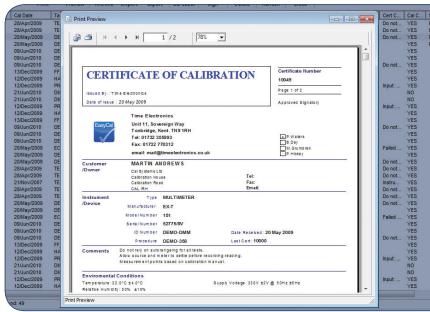

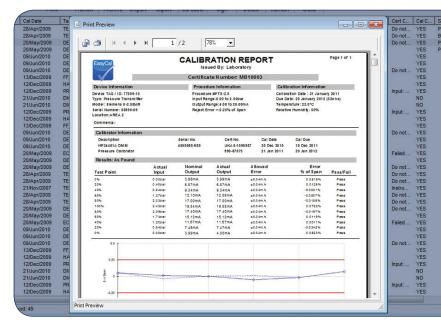


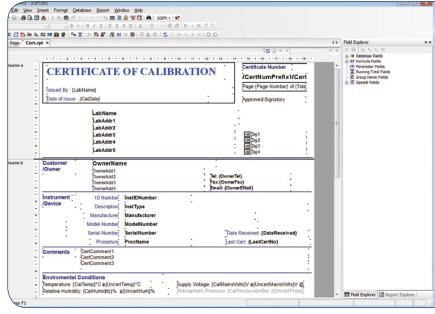




EasyCal Add-Ons and Accessories

Optional enhancements and extras for increased functionality

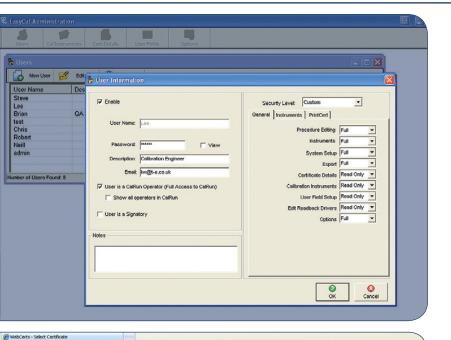

WebCerts Customer: SGE LTD Return to Customer List To reduce the number of certificates listed, enter one or more search critera below Cal Date Search Cert Num Inst ID 10003 WSE768 27/11/2007 DECADE BOX TIME 1051 9885F3 SGE LTD 25/11/2008 GE LTD 26/11/2008 10005 28/11/2007 FREQUENCY GENERATOR WSE752 BK PRECISION 3003 1585204 SGE LTD 26/11/2008 28/11/2007 MULTI FUNCTION CALIBRATOR SGE LTD 26/11/2008 10007 WSE777 12W730730 GE LTD 25/11/2008 0012 WSE784 28/11/2007 MULTIMETER YOKOGAWA 73303 1500940 SGE LTD 26/11/2008 GE LTD 26/11/2008 013 0014 WSE752 28/11/2007 FREQUENCY GENERATOR BK PRECISIO R&D SGE LTD 26/11/2008 3003 1585204 28/11/2007 MULTI FUNCTION CALIBRATO SGE LTD 26/11/2008 0016 WSE777 YOKOGAWA CA100 12W73073 29/11/2007 DIGITAL PRESSURE INDICATO ST74399 SGE LTD 27/11/2008 10023 040310735 30/11/2007 MULTIMETER METERMAN 37XR 040310735 SGE LTD 28/11/2008 03/12/2007 DIGITAL PRESSURE INDICATOR DRUCK ST74301 DPI705(IS) 7469/00+06 SGE LTD 01/12/2008 77 III MULTIMETER FLUKE GE LTD 02/12/2008

91G741417 728 04/12/2007 PRESSURE TRANSMITTER

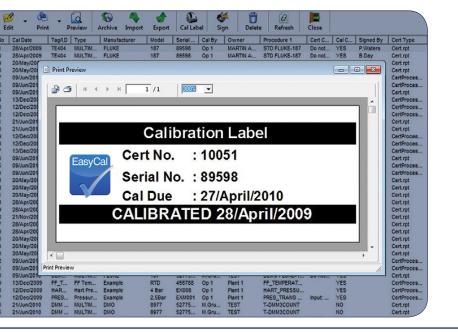

EJA110A

91G741417 728

EasyAdmin

EasyAdmin is an add-on that provides increased security for EasyCal and it's users.

User Rights: A master user sets the user rights for the relative staff and defines log in criteria.

Access Levels: Setting access levels within EasyCal to limit secondary users can be done, safe guarding sensitive information.

Administration: EasyAdmin provides an administration point for calibration instruments, certificate information and user fields.

Predefined Pick-Up Lists: For instrument manufacturers, sub contractors, customer details and other information. These can be created to make EasyCal data entry quick, easy and uniformed.

WebCerts

WebCerts is a web based application that enables EasyCal users to upload and retrieve certificates and reports online.

Simple Upload/Download: Uploading is incorporated into EasyCal by allowing the user to quickly and directly upload to their WebCert folders via FTP.

Secure User Log In: A security feature that allows users to access private folders with their relevant documentation. Ideal for companies with different sites or locations.

Search and Filter: Users can easily locate required data by using the filter tabs or the straightforward search fields.

Hosted Package: Time Electronics also offer a hosted WebCerts package where data is uploaded and stored on one of our designated WebCert servers. Retrieval and viewing of certificates is via the web based interface.

EasyCal Accessories

To complement and further optimise the calibration process Time Electronics offer a range of external options.

Printer and Connectivity Kit: Inkjet printer for calibration certificates and reports. Also includes a DVD-RW, 4 port USB hub, numeric key pad and USB memory stick.

Calibration and ID Label Printer: For printing labels to be placed on calibrated units. EasyCal has different layouts for required information to be shown.

Job and Address Label Printer: For printing information that accompanies a unit under test through the calibration process. Also for user tagging instruments.

Bar Code Reader: Enables fast identification of devices in the pre-calibration stage.

EasyCal to PC Communication Options: Interface cables and adaptors providing PC connectivity to Time Electronics calibrators or external instruments.

SGE LTD 02/12/2008

EasyCal Networking

With networking capabilities a multi-user system can be implemented




Networking with EasyCal

For multi-user systems EasyCal can be implemented as the universal software for administration, management, and control. With designated features for use in different workstations, EasyCal can provide a solution to calibration businesses with customers as well calibration departments within industrial plants.

Data can be shared and accessed on a central server, creating an organised and efficient networking set-up. EasyCal's pre-calibration features enable automated scheduling and also speed up the booking in process with quick instrument identification.

Calibration runs can be automated by using a compatible Time Electronics calibrator with EasyCal. Once calibration has been performed the data can be made available on the server to the necessary parties. Hard copy certificates and reports can be issued by authorised staff.

Enhanced security features can be added for increased protection, allowing a master user to control access rights to data and applications. Also available is an online application enabling users to upload and retrieve certificates.

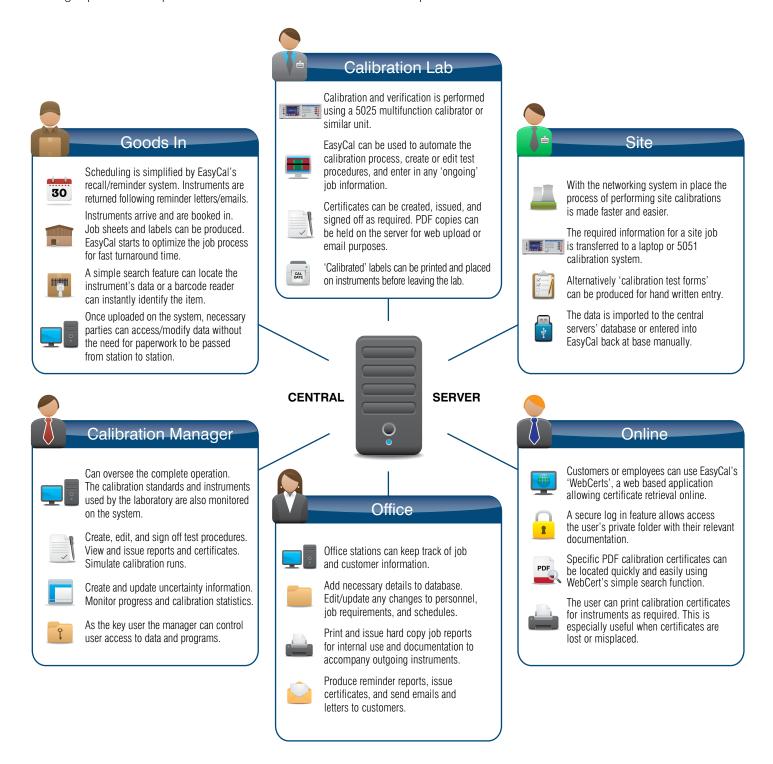

Comments Environments Failed on 3.2kOhm Measure Environments Environments Environments Failed on 3.2kOhm Measure Environments Environments Environments Failed on 3.2kOhm Measure Environments Environments Failed on 3.2kOhm Measure Environments Environments Environments Environments Failed on 3.2kOhm Measure Environments Environments Environments Environments Environments Environments Failed on 3.2kOhm Measure Environments Environ	CERTIFI	ICATE C	F CALIBRAT	ION	Certificate Number DM10005
Time Electronics Unit 11 Sovereign Way Tonbridge, Kent. TN9 1RH Tel: 01732 355993 Fax: 01732 770312 email: mail@timeelectronics.co.uk Customer Cal Systems Cultitude Unit 34 Lock Drive Unit 34 Lock Drive Unit 34 Lock Drive Unit 34 Lock Drive Sevenoaks Fax: Email: mail@t-6.co.uk Instrument Type Process Calibrator Manufacturer Fluke Model Number 725 Serial Number 419456 ID Number EC4 Procedure FLUKE-725-AUTO Last Cert: 10034 Comments Failed on 3.2kOhm Measure Environmental Conditions Temperature: 22 0°C ±4.0°C Relative Humidity: 50% ±10% Traceability Information Instrument Description Serial No Cert No Cert No Cert No Cert No Cert No Cel Date Cel Da	Issued Bv · Time Fle	ectronics			Page 1 of 3
Unit 11 Sovereign Way Tonbridge, Kent. TN9 1RH Tel: 01732 355993 Fax: 01732 770312 email: mail@timeelectronics.co.uk Customer Owner Cal House Unit 34 Lock Drive Sevenoaks Kent Unit 34 Lock Drive Sevenoaks Kent Tel: 01732 355599 Sevenoaks Kent Type Process Calibrator Manufacturer Fluke Model Number 725 Serial Number 175 Serial Number 1745 Serial Number 175 Serial Number 176 Serial Number 176 Serial Number 177 Serial Serial Number 178 Supply Voltage: 230V ±2V @ 50Hz ±5Hz Relative Humidity: 50% ±10% Serial Number 178 Supply Voltage: 230V ±2V @ 50Hz ±5Hz Supply Voltage: 230V ±2V @ 50Hz S	_				Approved Signatory
Unit 11 Sovereign Way Tonbridge, Kent. TN9 1RH Tel: 01732 355993 Fax: 01732 770312 email: mail@timeelectronics.co.uk Customer Owner Cal House Unit 34 Lock Drive Sevenoaks Kent Unit 34 Lock Drive Sevenoaks Kent Tel: 01732 355559 Sevenoaks Kent Type Process Calibrator Device Manufacturer Fluke Model Number 725 Serial Number 1745 Serial Number 1745 Serial Number 1745 Serial Number 175 Serial Number 1764 ID Number 177 Serial Number 178 Supply Voltage: 230V ±2V @ 50Hz ±5Hz Relative Humidity: 50% ±10% Supply Voltage: 230V ±2V @ 50Hz ±5Hz Relative Humidity: 50% ±10% Supply Voltage: 230V ±2V @ 50Hz ±5Hz Relative Humidity: 50% ±10% Supply Voltage: 230V ±2V @ 50Hz ±5Hz Supply Voltage: 230V ±2V @ 50Hz Supply Voltage: 230V ±2		Time Fleetwee	.:		•
Sovereign Way Tonbridge, Kent. TN9 1RH Tel: 01732 355993 Fax: 01732 770312 email: mall@timeelectronics.co.uk Customer Cal Systems Owner Cal House Unit 34 Lock Drive Sevenoaks Kent Type Process Calibrator Manufacturer Fluke Model Number 725 Serial Number 419456 ID Number EC4 Date Received: 20 May 2009 Procedure FLUKE-725-AUTO Last Cert: 10034 Comments Failed on 3.2kOhm Measure Environmental Conditions Falled on 3.2kOhm Measure Environmental Conditions Falled on 3.2kOhm Measure Environmental Conditions Comments Comments Falled on 3.2kOhm Measure Environmental Conditions C	Face Cal		IICS		
Tel: 01732 355993 Fax: 01732 770312 email: mail@timeelectronics.co.uk Sig 2	EasyCal		1		
email: mail@timeelectronics.co.uk Customer Owner Cal Systems Owner Cal House Unit 34 Lock Drive Sevenoaks Kent Type Process Calibrator Device Manufacturer Fluke Model Number 725 Serial Number 419456 ID Number EC4 Date Received: 20 May 2009 Procedure FLUKE-725-AUTO Last Cert: 10034 Comments Failed on 3.2kOhm Measure Environmental Conditions Failed on 3.2kOhm Measure Environmental Conditions Failed on 3.2kOhm Measure Environmental Conditions Fraceability Information Instrument Description Serial No Cert No Cert No Cal Date Cal Due Cal Due Conditions Comments Environmental Conditions Environmental Con		Tonbridge, Ke	nt. TN9 1RH		
Environmental Conditions Failed on 3.2kOhm Measure Failed on 3.2kOhm Measure Envi		Tel: 01732 355	993 Fax: 01732 770312		
Cal House Unit 34 Lock Drive Sevenoaks Kent Tol: 01732 355559 Fax: Email: mail@t-e.co.uk Instrument Type Process Calibrator Device Manufacturer Fluke Model Number 725 Serial Number 419456 ID Number EC4 Date Received: 20 May 2009 Procedure FLUKE-725-AUTO Last Cert: 10034 Comments Failed on 3.2kOhm Measure Environmental Conditions Femperature: 22.0°C ±4.0°C Relative Humidity: 50% ±10% Environmental Conditions Fraceability Information Instrument Description Serial No Cert No Cal Date Cal Date Cal Due Research Relative Humidity: 50% ±10% Comments Environmental Conditions Fraceability Information Instrument Description Serial No Cert No Cal Date Cal Due Relative Humidity: 50% ±10% Comments Environmental Conditions Fraceability Information Instrument Description Serial No Cert No Cal Date Cal Due Relative Humidity: 50% ±10% Comments Comments Environmental Conditions Fraceability Information Instrument Description Serial No Cert No Cal Date Cal Due Relative Humidity: 50% ±10% Comments Fraceability Information Instrument Description Serial No Comments Comments Fraceability Information Instrument Description Serial No Cert No Cal Date Cal Due Relative Humidity: 50% ±10% Comments Fraceability Information Instrument Description Serial No Cert No Cal Date Relative Humidity: 50% ±10% Comments Fraceability Information Instrument Description Serial No Cert No Cal Date Relative Humidity: 50% ±10% Comments Fraceability Information Instrument Description Serial No Cert No Cal Date Relative Humidity: 50% ±10% Comments Fraceability Information Instrument Description Serial No Cert No Cal Date Relative Humidity: 50% ±10% Comments Fraceability Information Instrument Description Serial No Cert No Cal Date Relative Humidity: 50% ±10% Relative Humidity: 50% ±10% Relative Humidity: 50% ±10% Relative Humidity: 50% Relative Humid		email: mail@ti	meelectronics.co.uk		
Cal Problem Unit 34 Lock Drive Sevenoaks Kent Type Process Calibrator Device Manufacturer Fluke Model Number 725 Serial Number 419456 ID Number EC4 Date Received: 20 May 2009 Procedure FLUKE-725-AUTO Last Cert: 10034 Comments Failed on 3.2kOhm Measure Environmental Conditions Femperature: 22.0°C ±4.0°C Relative Humidity: 50% ±10% Fraceability Information Instrument Description Serial No Cert No Cal Date Cal Due 0825 May 2009 Or May 2010 Course: 50,400,200,400,400,400,400,400,400,400,40		Cal Systems	3		
Sevenoaks Kent Type Process Calibrator Manufacturer Fluke Model Number 725 Serial Number 419456 ID Number EC4 Date Received: 20 May 2009 Procedure FLUKE-725-AUTO Last Cert: 10034 Comments Failed on 3.2kOhm Measure Environmental Conditions Temperature: 22.0°C ±4.0°C Relative Humidity: 50% ±10% Serial No Cert No Supply Voltage: 230V ±2V @ 50Hz ±5Hz Relative Humidity: 50% ±10% Comments Serial No Cert No Cal Date Cal Due 5025 Multifunction Calibrator 108908 UKAS-90897 08 May 2009 07 May 2010 ac Current: 5pa. 400.44-40 5py. 1-106, 1000.24-24-04-1054-25my-2004-2004-04-055+-304, 120my-2004-055+-304, 120my-200	/Owner			T.1. 04800.00	
Rent Type Process Calibrator Device Manufacturer Fluke Model Number 725 Serial Number 419456 ID Number EC4 Date Received: 20 May 2009 Procedure FLUKE-725-AUTO Last Cert: 10034 Comments Failed on 3.2kOhm Measure Environmental Conditions Femperature: 22.0°C ±4.0°C Relative Humidity: 50% ±10% Environmental Conditions Fraceability Information Instrument Description Serial No Cert No Cal Date Cal Due (1965 Multifunction Calibrator 1089 G08 UKAS-90897 08 May 2009 07 May 2010 (1965 Multifunction Calibrator 1089 G08 UKAS-90897 08 May 2009 07 May 2010 (1965 Multifunction Calibrator 1089 G08 UKAS-90897 08 May 2009 07 May 2010 (1965 Multifunction Calibrator 1089 G08 UKAS-90897 08 May 2009 07 May 2010 (1965 Multifunction Calibrator 1089 G08 UKAS-90897 08 May 2009 07 May 2010 (1965 Multifunction Calibrator 1089 G08 UKAS-90897 08 May 2009 07 May 2010 (1965 Multifunction Calibrator 1089 G08 UKAS-90897 08 May 2009 07 May 2010 (1965 Multifunction Calibrator 1089 G08 UKAS-90897 08 May 2009 07 May 2010 (1965 Multifunction Calibrator 1089 G08 UKAS-90897 08 May 2009 07 May 2010 (1965 Multifunction Calibrator 1089 G08 UKAS-90897 08 May 2009 07 May 2010 (1965 Multifunction Calibrator 1089 G08 UKAS-90897 08 May 2009 07 May 2010 (1965 Multifunction Calibrator 1089 G08 UKAS-90897 08 May 2009 07 May 2010 (1965 Multifunction Calibrator 1089 G08 UKAS-90897 08 May 2009 07 May 2010 (1965 Multifunction Calibrator 1089 G08 UKAS-90897 08 May 2009 07 May 2010 (1965 Multifunction Calibrator 1089 G08 UKAS-90897 08 May 2009 07 May 2010 (1965 Multifunction Calibrator 1089 Multifunction Calibrator 1089 G08 Multifunction Calibrator 1089 G08 Multifunction Calibrator 108 Multifunction Calibrator 1089 G08 Multifunction Calibrator 1089 Multifunction Calibrator 1089 Multifunction Cal			ve .		5559
Manufacturer Fluke					t-e.co.uk
Manufacturer Fluke Model Number 725 Serial Number 419456 ID Number EC4 Date Received: 20 May 2009 Procedure FLUKE-725-AUTO Last Cert: 10034 Comments Failed on 3.2kOhm Measure Environmental Conditions Temperature: 22.0°C ±4.0°C Supply Voltage: 230V ±2V @ 50Hz ±5Hz Relative Humidity: 50% ±10% Fraceability Information Instrument Description Serial No Cert No Cal Date Cal Due 0 May 2009 0 7 May 2010 Courrent EpA-200uA-0 37%-3800A(200uA-2mA-0.05%-300A(20mA-205%-300A(20mA-0.05%-300A(20mA-20-0.0%-0.0%-300A(200mA-20-0.0%-300A(20mA-20-0.0%-300A(200mA-200MA-300A(200mA-200MA-300A(200mA-200MA-300A(200mA-200MA-300A(200mA-200MA-300MA-300MA-300MA-300MA-300MA-300MA-300MA-300A(200mA-200MA-300MA-300A(200mA-200MA-300M		Туре	Process Calibrator		
Serial Number	Device	Manufacturer	Fluke		
ID Number EC4		Model Number	725		
Procedure FLUKE-725-AUTO Last Cert: 10034		Serial Number	419456		
Enviromental Conditions Temperature: 22.0°C ±4.0°C Supply Voltage: 230V ±2V @ 50Hz ±5Hz Relative Humidity: 50% ±10% Fraceability Information Instrument Description Serial No Cert No Cal Date Cal Due 1025 Multifunction Calibrator 1089G08 UKAS-90897 08 May 2009 07 May 2010 10 Current: 9pA-200uA-9 07%+390nAj200uA-2mA-9.05%+390nAj2mA-20mA-0.65%+3uAj20mA-20mA-0.05%+30uAj20mA-2A-0.15%+0.5mAj2A-20A-0.2%+5mAj 10 Cvoltage: 1mV-20mV-0.05%+256uVj20mV-200mV-0.04%+150uV (45Hz-10kHz)]200mV-2V-0.03%+256uV (45Hz-10kHz)]2V-20V-0.03%+3mV (45H		ID Number	EC4	Date Received: 20 N	lay 2009
Enviromental Conditions Temperature: 22.0°C ±4.0°C Supply Voltage: 230V ±2V @ 50Hz ±5Hz Relative Humidity: 50% ±10% Fraceability Information Instrument Description Serial No Cert No Cal Date Cal Due 1025 Multifunction Calibrator 1089G08 UKAS-90897 08 May 2009 07 May 2010 10 Current: 9pA-200uA-9 07%+390nAj200uA-2mA-9.05%+390nAj2mA-20mA-0.65%+3uAj20mA-20mA-0.05%+30uAj20mA-2A-0.15%+0.5mAj2A-20A-0.2%+5mAj 10 Cvoltage: 1mV-20mV-0.05%+256uVj20mV-200mV-0.04%+150uV (45Hz-10kHz)]200mV-2V-0.03%+256uV (45Hz-10kHz)]2V-20V-0.03%+3mV (45H					
Cert No	Comments Fa			Last Cert: 10034	
Traceability Information Instrument Description Serial No Cert No Cal Date Cal Due 5025 Multifunction Calibrator 1089G08 UKAS-90897 08 May 2009 07 May 2010 AC Current: 0pA-200uA=0.07%+300nA 200uA-2mA=0.05%+300nA 2mA-20mA=0.05%+30uA 20mA-20mA=0.05%+30uA 20mA-2A=0.1%+0.5mA 2A-20A=0.2%+5mA AC Voltage: 1mV-20mV=0.05%+250uV 20mV-20mV=0.04%+150uV (45Hz-10kHz) 20vmV-2V=0.03%+250uV (45Hz-10kHz) 2V-20V=0.03%+3mV (45Hz-10kHz) 2V-20V=0.05%+30uA 20mA-20mA=0.05%+30uA 20mA-2A=0.05%+30uA 20mA	Enviromental Condi	ailed on 3.2kOhm M	leasure		50U +5U
Serial No Cert No Cal Date Cal Due	Enviromental Condi Temperature: 22.0°C :	ailed on 3.2kOhm M itions ±4.0°C	leasure		50Hz ±5Hz
1089G8 UKAS-90897 08 May 2009 07 May 2010	Enviromental Condi Temperature: 22.0°C : Relative Humidity: 50%	ailed on 3.2kOhm M itions ±4.0°C % ±10%	leasure		50Hz ±5Hz
AC Voltage: :mV-20mV=0.05%+259uV 20mV-200mV=0.04%+150uV (45Hz-10kHz) 200mV-2V=0.03%+250uV (45Hz-10kHz) 2V-20V=0.03%+35mV (45Hz-10kHz) 20V-200V=0.06%+20mV 20V-1.05kV=0.08%+290mV DC Current: 0pA-200uA=150ppm+15nA 200uA-2mA=100ppm+40nA 2mA-20mA=80ppm+200nA 20mA-20mA=80ppm+3uA 200mA-2A=250ppm+40uA 2A-20A=600ppm+2mA DC Current: 0pA-200uA=150ppm+4uV 20mV-200mV=30ppm+6uV 200mV-2V=15ppm+20uV 2V-2V=15ppm+15uV 20V-200V=30ppm+6mV 200V-1.05kV=50ppm+30mV DC Urrent: 0pA-200uA=100ppm+4uV 20mV-200mV=30ppm+6uV 200mV-2V=15ppm+20uV 2V-20V=30ppm+6mV 200V-1.05kV=50ppm+30mV DC Urrent: 0pA-200uA=100ppm+4uV 20mV-200mV=30ppm+6uV 200mV-2V=15ppm+20uV 2V-20V=30ppm+6mV 200V-1.05kV=50ppm+30mV DC Urrent: 0pA-200uA=0.07%+300nA 20uA-2mA=0.05%+30uA 20mA-200mA=0.05%+30uA 20mA-2A=0.1%+0.5mA 2A-20A=0.2%+5mA CC Voltage: 1mV-20mV=0.05%+250uV 20mV-20mV=0.04%+150uV (45Hz-10kHz) 20V-20V=0.03%+250uV (45Hz-10kHz) 2V-2V=0.03%+3mV (45Hz-10kHz) 2V-2V=0.05%+250ppm+3mV DC Urrent: 0pA-200uA=150ppm+15nA 200uA-2mA=100ppm+40nA 2mA-20mA=90pm+20uA 2mA-200mA=0ppm+3uA 20mA-2A=250ppm+40uA 2A-20A=600ppm+2mA DC Voltage: 0pV-20mV=10ppm+40uV 20mV-200mV=20ppm+40uV 20mV-20mV=30ppm+40uV 20mV-200mV=30pmV	Enviromental Condi Temperature: 22.0°C : Relative Humidity: 50% Traceability Informa	itions ±4.0°C % ±10%	leasure Supp	ply Voltage: 230V ±2V @	
DC Current: 0pA-200iuA=150ppm+15nA]200uA-2mA=100ppm+40nA]2mA-20mA=80ppm+20uA]20mA-200nA=80ppm+3uA]20mA-2-250ppm+40uA]2A-20A=800ppm+2mA] DC Voltage: 0pV-20mV=100ppm+4uV 20mV-20mV=30ppm+6uV 200mV-2V=15ppm+20uV 2V-20V=15ppm+150uV 20V-200V=30ppm+6mV 200V-1.05kV=50ppm+30mV Resistance: 0pR-1002=0.01%+7mQ 10002-1kQ=0.01%+5mQ 1kQ=0.02%+20mQ 10kQ-1.00kQ=0.01%+1Q 10kQ-1MQ=0.01%+1Q 10kQ-1MQ=0.02%+100mQ 10MQ-1.20MQ=0.1%+1kQ 5075 Digital Multimeter 109PC4 39803 19 May 2009 18 May 2010 AC Current: 0pA-200uA=0.07%+300nA 20uA-2mA=0.65%+30uA 20mA-2.00mA=0.65%+30uA 20mA-2A=0.1%+0.5mA]2A-20A=0.2%+5mA AC Voltage: 1mW-20mV=0.05%+250uV 20mV-20uV=0.04%+150uV (45Hz-10kHz) 20V=0.03%+250uV (45Hz-10kHz) 2V-2V=0.03%+3mV (45Hz-10kHz) 2V=0.03%+3mV (45H	Enviromental Condi Temperature: 22.0°C: Relative Humidity: 50% Traceability Informa Instrument Description	itions ±4.0°C % ±10%	leasure Supp Cert No	ply Voltage: 230V ±2V @ Cal Date	Cal Due
Resistance: 0pR-1000=0.01%+7mQ 1000_1kQ=0.01%+5mQ 1kQ-10kQ=0.02%+20mQ 10kQ-100kQ=0.01%+10Q 100kQ-1MQ=0.01%+10Q 1MQ-10MQ=0.02%+100mQ 10MQ-120MQ=0.1%+1kQ \$075 Digital Multimeter	Enviromental Condi Temperature: 22.0°C: Relative Humidity: 50% Traceability Informa Instrument Description 5025 Multifunction Calibrat Ac Current: 0pA-200uA=0.07%+300 Ac Voltage: 1mV-20mV=0.05%+2500	itions ±4.0°C % ±10% ation Serial No tor 1089G08 http://doi.org/10.000/10.2004-2mA=0.05%-300nAj	Cert No UKAS-90897 2mA-20mA=0.05%+3uA 20mA=0.05%+30uA 20	ply Voltage: 230V ±2V @ <i>Cal Date</i> 08 May 2009	<i>Cal Due</i> 0 07 May 2010
AC Current: 0pA-200uA=0.07%+300nA 200uA-2mA=0.05%+300nA 2mA-20mA=0.05%+3uA 20mA-200mA=0.05%+30uA 200mA-24=0.1%+0.5mA 2A-20A=0.2%+5mA AC Voltage: 1mV-20mV=0.05%+259uV 20mV-200mV=0.04%+150uV (45Hz-10kHz) 200mV-2V=0.03%+250uV (45Hz-10kHz) 2V-20V=0.03%+3mV (45Hz-10kHz) 2V-20V=0.03%+3mV (45Hz-10kHz) 2V-20V=0.03%+3mV (45Hz-10kHz) 2V-20V=0.03%+3mV (45Hz-10kHz) 2V-20V=0.03%+3mV (45Hz-10kHz) 2V-20V=0.05%+30mV 200V=0.05%+30mV 200V=0.05	Enviromental Condi Temperature: 22.0°C: Relative Humidity: 50% Traceability Informa instrument Description 5025 Multifunction Calibral AC Current: 0pA-200uA=0.07%+300 AC Voltage: 1mV-20mV=0.05%+250. 0.05kV=0.08%+90mV] 0.05kV=0.08%+90mV]	itions ±4.0°C % ±10% ation Serial No tor 1089908 Ina 200uA-2mA=0.05%-300nA uV 20mV=0.04%+150uV 5nA 200uA-2mA=100ppm+40nV	Cert No	Cal Date 08 May 2009 000mA-2A=0.1%+0.5mA 2A-20A=0.2%+5m 0)2V-20V=0.03%+3mV (45Hz-10kHz) 20V-2	<i>Cal Due</i> 07 May 2010 tA :00∨=0.06%+20mV 200V- 0ppm+2mA
C Voltage: 1mV-20mV=0.05%+250uV 20mV-200mV=0.04%+150uV (45Hz-10kHz) 200mV-2V=0.03%+250uV (45Hz-10kHz) 2V-20V=0.03%+3mV (45Hz-10kHz) 20V-200V=0.06%+20mV 200V-0.05%+00mV .05KV=0.05%+09mV C Current: 0pA-200uA=150ppm+15nA 200uA-zmA=100ppm+40nA 2mA-20mA=80ppm+200nA 20mA-200mA=80ppm+3uA 200mA-2A=250ppm+40uA 2A-20A=600ppm+2mA C Voltage: 0pV-20mV=100ppm+4uV 20mV-200mV=30ppm+6uV 200mV-2V=15ppm+20uV 2V-20V=15ppm+150uV 20V-200V=30ppm+6mV 200V-1.05KV=50ppm+30mV	Enviromental Condi Γemperature: 22.0°C: Relative Humidity: 50% Fraceability Informa Instrument Description 6025 Multifunction Calibrat 6.0 Current: 0pA-200uA=0.07%+300 6.0 Current: 0pA-200uA=450ppm+41 6.0 Current: 0pA-200uA=150ppm+41 6.0 Voltage: 0pV-20mV-100ppm+4u tesistance: 0pR-1000=0.01%+7mΩl	itions ±4.0°C % ±10% ation Serial No tor 1089G08 ana 200uA-2mA=0.05%+300nA u/y 20mV-200mV=30ppm+40n u/y 20mV-20pm+50ppm+60v 20mV 20mV=20ppm+60v 20mV=0.04%+50v 40mV 20mV=0.04%+50v 40mV=0.00mV=0.04%+50v 40mV=0.04%+50v 40mV=0.04%+	Cert No	Cal Date 08 May 2009 100mA-2A=0.11%+0.5mA 2A-20A=0.2%+5m 101V-3209-0.3%+3mV (α8Hz-10kHz) 200-4.00%+3mV (α8Hz-10kHz) 200+1.05kV=50ppm+3 101=0.01%+10Ω 1MΩ-10MΩ=0.02%+100mΩ	Cal Due 07 May 2010 IA] 100V=0.06%+20mV 200V- 00ppm+2πA 0mV □ 10MΩ-120MΩ=0.1%+1kΩ
DC Voltage: 0pV-20mV=100ppm+4uV 20mV-200mV=30ppm+6uV 200mV-2V=15ppm+20uV 2V-20V=15ppm+150uV 20V-200V=30ppm+6mV 200V-1.05kV=50ppm+30mV	Enviromental Condi Temperature: 22.0°C: Relative Humidity: 50° Traceability Informa Instrument Description 5025 Multifunction Calibrat AC Current: 0pA-200uA=0.07%+300. AC Voltage: 1mV-20mV=0.05%+250i. LoStv=0.08%+90mV DC Current: 0pA-200uA=150ppm+1t UC Voltage: 0pV-20mV=100ppm+20 UC Voltage: 0pV-20mV=100ppm+20 To Voltage: 0pV-20mV=100ppm+	itions ±4.0°C % ±10% ation Serial No tor 1089G08 http://doi.org/10.0004/2mA=100ppm+40nu/1/20mV-200mV=30ppm+6uV/1/21 1000-1kD=0.01%+5mD 1kD-0.01%+5mD 1kD-	Cert No UKAS-90897 2mA-20mA=0.05%+3uA 20mA-20mA=0.05%+30uA 2 ((45Hz-10kHz) 200mV-2V=0.03%+256uV (45Hz-10kHz 4)2mA-20mA=80ppm+200mA 20mA-20mA=80ppm+3 00vV-2V=15ppm+50uV 2V-20V=15ppm+150uV 20V-2 k\Omega=0.02%+20m\Omega 10k\Omega=0.01%+1\Omega 100k\Omega=0.01%+1\Omega 100k\Omega=0.01%+1\Omega=0.01%+1\Omega=0.02%+20m\Omega=0.01%+1\Omega=0.	Cal Date 08 May 2009 100mA-2A=0.1%+0.5mA 2A-20A=0.2%+5m 2V-20V=0.03%+3mV (45Hz-10kHz) 20V-2 uLα 200mA-2A=250ppm+6uLα 2A-20A=0 00V=30ppm+6mV 200V-1.05kV=50ppm+3 00V=30pym+6mV 200V-1.05kV=50ppm+3 19 May 2009	Cal Due 07 May 2010 iA :000V=0.06%+20mV 200V- 0ppm+2mA 0mV i 10MΩ-120MΩ=0.1%+1kΩ 18 May 2010
	Enviromental Condi Temperature: 22.0°C: Relative Humidity: 50% Traceability Informa Instrument Description 5025 Multifunction Calibral AC Current: 0pA-200uA=0.07%+300 AC Current: 0pA-200uA=150ppm+12 0C Current: 0pA-200uA=150ppm+12 DC Voltage: 0pV-20mV-100ppm+4u Resistance: 0pR-10002=0.01%+7mQi 5075 Digital Multimeter AC Current: 0pA-200uA=0.07%+300 AC Voltage: 1mV-20mV-0.05%+2501	itions	Cert No UKAS-90897 2mA-20mA=0.05%+3uA 20mA-20mA=0.05%+30uA 2 (145Hz-10kHz) 200mV-2V=0.03%+256uV (45Hz-10kHz 2)2mA-20mA=80ppm+200nA 20mA-200mA=80ppm+300mV-2V=0.05%+20mU 20V-20V-20V=0.05%+20mU 10kΩ-10kΩ=0.01%+10 10kΩ-1M	Cal Date 08 May 2009 100mA-2A=0.1%+0.5mA 2A-20A=0.2%+5m 2V-20V=0.03%+3mV (45Hz-10kHz) 20V-200pm+6mV 200V-1.05kV=50ppm+3 10=0.01%+10Ω 1MΩ-10MΩ-0.02%+5m 3P May 2008 100mA-2A=0.1%+0.5mA 2A-20A=0.2%+5m 2V-20V=0.03%+3mV (45Hz-10kHz) 20V-2	Cal Due 07 May 2010 IA 1000V=0.06%+20mV 200V- 0ppm+2mA 0mV 1 100MΩ-120MΩ=0.1%+1kΩ 18 May 2010 IA 100V=0.06%+20mV 200V-
Resistance: 0pR-100 Ω =0.01%+7m Ω 100 Ω -1k Ω =0.01%+5m Ω 1k Ω -10k Ω =0.02%+20m Ω 10k Ω -100k Ω =0.01%+1 Ω 100k Ω -1M Ω =0.01%+10 Ω 1M Ω -10M Ω =0.02%+100m Ω 10M Ω -120M Ω =0.1%+1k Ω	Enviromental Condi Temperature: 22.0°C: Relative Humidity: 50°C: Relative Humidity: 50°C: Traceability Informal Instrument Description S025 Multifunction Calibrat AC Current: 0pA-200uA=0.07%+300 AC Voltage: 1mV-20mV=0.05%+250: 1.08KV=0.08%+90mV] COURTEN: 0pA-200uA=150ppm+10 Resistance: 0pR-1009=0.01%+7 AC Current: 0pA-200uA=0.07%+300 AC Voltage: 1mV-20mV=0.05%+250: 1.08KV=0.08%+90mV] DC Current: 0pA-200uA=150ppm+10 CC Voltage: 0pV-20mV=100ppm+410 COURDENTENTENTENTENTENTENTENTENTENTENTENTENTE	itions ±4.0°C % ±10% ation Serial No tor 1089G08 InA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV 5nA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV 5nA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV 5nA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV	Cert No	Cal Date 08 May 2009 100mA-2A=0.1%+0.5mA]2A-20A=0.2%+5m 102V-20V=0.03%+3mV (45Hz-10kHz)]20V-2 1020mA-2A=0.19m-0.10M20-0.02%+100m 109-0.09%+100µ1MΩ-1.08M20-0.2%+5m 19 May 2009 100mA-2A=0.1%+0.5mA]2A-20A=0.2%+5m 1)2V-20V=0.03%+3mV (45Hz-10kHz)]20V-2 100mA-2A=0.1%+0.5mA]2A-20A=0.00%+30pm+6mV]20V-20V-20V-200-0.03%+3mV (45Hz-10kHz)]20V-20V-20V-2009m+6mV]20V-20V-20V-2009m+6mV]20V-200V-1.05kV-50ppm+3	Cal Due 07 May 2010 IA 100V=0.06%+20mV 200V- 0ppm+2mA 0mV 1 10MΩ-120MΩ=0.1%+1kΩ 18 May 2010 IA 100V=0.06%+20mV 200V- 0ppm+2mA 0mV
	Enviromental Condi Temperature: 22.0°C: Relative Humidity: 50°C: Relative Humidity: 50°C: Traceability Informal Instrument Description S025 Multifunction Calibrat AC Current: 0pA-200uA=0.07%+300 AC Voltage: 1mV-20mV=0.05%+250: 1.08KV=0.08%+90mV] COURTEN: 0pA-200uA=150ppm+10 Resistance: 0pR-1009=0.01%+7 AC Current: 0pA-200uA=0.07%+300 AC Voltage: 1mV-20mV=0.05%+250: 1.08KV=0.08%+90mV] DC Current: 0pA-200uA=150ppm+10 CC Voltage: 0pV-20mV=100ppm+410 COURDENTENTENTENTENTENTENTENTENTENTENTENTENTE	itions ±4.0°C % ±10% ation Serial No tor 1089G08 InA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV 5nA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV 5nA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV 5nA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV	Cert No	Cal Date 08 May 2009 100mA-2A=0.1%+0.5mA]2A-20A=0.2%+5m 102V-20V=0.03%+3mV (45Hz-10kHz)]20V-2 1020mA-2A=0.19m-0.10M20-0.02%+100m 109-0.09%+100µ1MΩ-1.08M20-0.2%+5m 19 May 2009 100mA-2A=0.1%+0.5mA]2A-20A=0.2%+5m 1)2V-20V=0.03%+3mV (45Hz-10kHz)]20V-2 100mA-2A=0.1%+0.5mA]2A-20A=0.00%+30pm+6mV]20V-20V-20V-200-0.03%+3mV (45Hz-10kHz)]20V-20V-20V-2009m+6mV]20V-20V-20V-2009m+6mV]20V-200V-1.05kV-50ppm+3	Cal Due 07 May 2010 IA 100V=0.06%+20mV 200V- 0ppm+2mA 0mV 1 10MΩ-120MΩ=0.1%+1kΩ 18 May 2010 IA 000V=0.06%+20mV 200V- 00ppm+2mA 0mV
	Enviromental Condi Temperature: 22.0°C: Relative Humidity: 50°C: Relative Humidity: 50°C: Fraceability Informa Instrument Description S025 Multifunction Calibrat AC Current: 0pA-200uA=0.07%+250. JOSEA DO. 80%+90mV DC Voltage: 1mV-20mV=0.05%+250. S050-100-100-100-100-100-100-100-100-100-	itions ±4.0°C % ±10% ation Serial No tor 1089G08 InA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV 5nA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV 5nA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV 5nA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV	Cert No	Cal Date 08 May 2009 100mA-2A=0.1%+0.5mA]2A-20A=0.2%+5m 102V-20V=0.03%+3mV (45Hz-10kHz)]20V-2 1020mA-2A=0.19m-0.10M20-0.02%+100m 109-0.09%+100µ1MΩ-1.08M20-0.2%+5m 19 May 2009 100mA-2A=0.1%+0.5mA]2A-20A=0.2%+5m 1)2V-20V=0.03%+3mV (45Hz-10kHz)]20V-2 100mA-2A=0.1%+0.5mA]2A-20A=0.00%+30pm+6mV]20V-20V-20V-200-0.03%+3mV (45Hz-10kHz)]20V-20V-20V-2009m+6mV]20V-20V-20V-2009m+6mV]20V-200V-1.05kV-50ppm+3	Cal Due 07 May 2010 IA 100V=0.06%+20mV 200V- 0ppm+2mA 0mV 1 10MΩ-120MΩ=0.1%+1kΩ 18 May 2010 IA 100V=0.06%+20mV 200V- 00ppm+2mA 0mV
	Enviromental Condi Temperature: 22.0°C: Relative Humidity: 50°C: Relative Humidity: 50°C: Fraceability Informa Instrument Description S025 Multifunction Calibrat AC Current: 0pA-200uA=0.07%+250. JOSEA DO. 80%+90mV DC Voltage: 1mV-20mV=0.05%+250. S050-100-100-100-100-100-100-100-100-100-	itions ±4.0°C % ±10% ation Serial No tor 1089G08 InA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV 5nA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV 5nA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV 5nA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV	Cert No	Cal Date 08 May 2009 100mA-2A=0.1%+0.5mA]2A-20A=0.2%+5m 102V-20V=0.03%+3mV (45Hz-10kHz)]20V-2 1020mA-2A=0.19m-0.10M20-0.02%+100m 109-0.09%+100µ1MΩ-1.08M20-0.2%+5m 19 May 2009 100mA-2A=0.1%+0.5mA]2A-20A=0.2%+5m 1)2V-20V=0.03%+3mV (45Hz-10kHz)]20V-2 100mA-2A=0.1%+0.5mA]2A-20A=0.00%+30pm+6mV]20V-20V-20V-200-0.03%+3mV (45Hz-10kHz)]20V-20V-20V-2009m+6mV]20V-20V-20V-2009m+6mV]20V-200V-1.05kV-50ppm+3	Cal Due 07 May 2010 IA 100V=0.06%+20mV 200V- 0ppm+2mA 0mV 1 10MΩ-120MΩ=0.1%+1kΩ 18 May 2010 IA 100V=0.06%+20mV 200V- 0ppm+2mA 0mV
	Enviromental Condi Temperature: 22.0°C: Relative Humidity: 50°C: Relative Humidity: 50°C: Fraceability Informa Instrument Description S025 Multifunction Calibrat AC Current: 0pA-200uA=0.07%+250. JOSEA DO. 80%+90mV DC Voltage: 1mV-20mV=0.05%+250. S050-100-100-100-100-100-100-100-100-100-	itions ±4.0°C % ±10% ation Serial No tor 1089G08 InA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV 5nA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV 5nA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV 5nA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV	Cert No	Cal Date 08 May 2009 100mA-2A=0.1%+0.5mA]2A-20A=0.2%+5m 102V-20V=0.03%+3mV (45Hz-10kHz)]20V-2 1020mA-2A=0.19m-0.10M20-0.02%+100m 109-0.09%+100µ1MΩ-1.08M20-0.2%+5m 19 May 2009 100mA-2A=0.1%+0.5mA]2A-20A=0.2%+5m 1)2V-20V=0.03%+3mV (45Hz-10kHz)]20V-2 100mA-2A=0.1%+0.5mA]2A-20A=0.00%+30pm+6mV]20V-20V-20V-200-0.03%+3mV (45Hz-10kHz)]20V-20V-20V-2009m+6mV]20V-20V-20V-2009m+6mV]20V-200V-1.05kV-50ppm+3	Cal Due 07 May 2010 IA 100V=0.06%+20mV 200V- 0ppm+2mA 0mV 1 10MΩ-120MΩ=0.1%+1kΩ 18 May 2010 IA 100V=0.06%+20mV 200V- 00ppm+2mA 0mV
	Enviromental Condi Temperature: 22.0°C: Relative Humidity: 50°C: Relative Humidity: 50°C: Fraceability Informa Instrument Description S025 Multifunction Calibrat AC Current: 0pA-200uA=0.07%+250. JOSEA DO. 80%+90mV DC Voltage: 1mV-20mV=0.05%+250. S050-100-100-100-100-100-100-100-100-100-	itions ±4.0°C % ±10% ation Serial No tor 1089G08 InA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV 5nA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV 5nA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV 5nA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV	Cert No	Cal Date 08 May 2009 100mA-2A=0.1%+0.5mA]2A-20A=0.2%+5m 102V-20V=0.03%+3mV (45Hz-10kHz)]20V-2 1020mA-2A=0.19m-0.10M20-0.02%+100m 109-0.09%+100µ1MΩ-1.08M20-0.2%+5m 19 May 2009 100mA-2A=0.1%+0.5mA]2A-20A=0.2%+5m 1)2V-20V=0.03%+3mV (45Hz-10kHz)]20V-2 100mA-2A=0.1%+0.5mA]2A-20A=0.00%+30pm+6mV]20V-20V-20V-200-0.03%+3mV (45Hz-10kHz)]20V-20V-20V-2009m+6mV]20V-20V-20V-2009m+6mV]20V-200V-1.05kV-50ppm+3	Cal Due 07 May 2010 IA 100V=0.06%+20mV 200V- 0ppm+2mA 0mV 1 10MΩ-120MΩ=0.1%+1kΩ 18 May 2010 IA 100V=0.06%+20mV 200V- 0ppm+2mA 0mV
	Enviromental Condi Temperature: 22.0°C: Relative Humidity: 50°C: Relative Humidity: 50°C: Traceability Informal Instrument Description S025 Multifunction Calibrat AC Current: 0pA-200uA=0.07%+300. AC Voltage: ImV-20mV=0.05%+250. Current: 0pA-200uA=150ppm+10 Courrent: 0pA-200uA=0.07%+300. Current: 0pA-200uA=0.07%+300. Current: 0pA-200uA=0.07%+300. Current: 0pA-200uA=0.07%+300. Current: 0pA-200uA=0.07%+300. Current: 0pA-200uA=150ppm+10. Current: 0pA-200uA=150ppm+10. Current: 0pA-200uA=150ppm+10. Current: 0pA-200uA=150ppm+10. Current: 0pA-200uA=150ppm+10. Current: 0pA-200uA=150ppm+11.	itions ±4.0°C % ±10% ation Serial No tor 1089G08 InA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV 5nA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV 5nA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV 5nA 200uA-2mA=0.05%-300nA uV 20mV-200mV=0.04%+150uV	Cert No	Cal Date 08 May 2009 100mA-2A=0.1%+0.5mA]2A-20A=0.2%+5m 102V-20V=0.03%+3mV (45Hz-10kHz)]20V-2 1020mA-2A=0.19m-0.10M20-0.02%+100m 109-0.09%+100µ1MΩ-1.08M20-0.2%+5m 19 May 2009 100mA-2A=0.1%+0.5mA]2A-20A=0.2%+5m 1)2V-20V=0.03%+3mV (45Hz-10kHz)]20V-2 100mA-2A=0.1%+0.5mA]2A-20A=0.00%+30pm+6mV]20V-20V-20V-200-0.03%+3mV (45Hz-10kHz)]20V-20V-20V-2009m+6mV]20V-20V-20V-2009m+6mV]20V-200V-1.05kV-50ppm+3	Cal Due 07 May 2010 IA 100V=0.06%+20mV 200V- 0ppm+2mA 0mV 1 10MΩ-120MΩ=0.1%+1kΩ 18 May 2010 IA 100V=0.06%+20mV 200V- 0ppm+2mA 0mV
Calibrated by: Robert Martins Date of Calibration: 20 May 2009 Calibration Due: 19 May 2	Enviromental Condi Temperature: 22.0°C: Relative Humidity: 50°C: Relative Humidity: 50°C: Traceability Informa instrument Description Co25 Multifunction Calibrat AC Current: 0pA-200uA=0.07%+300 AC Voltage: imV-20mV=0.05%+2501 DC Voltage: 0pV-20mV=100ppm+41 DC Voltage: 0pV-20mV=100ppm+40 Environt: 0pA-200uA=0.07%+300 AC Voltage: imV-20mV=0.05%+2501 L05kV=0.08%+90mV] DC Current: 0pA-200uA=150ppm+10 DC Current: 0pA-200uA=150ppm+10 DC Voltage: 0pV-20mV=100ppm+44 Resistance: 0pR-1000=0.01%+7mQ Resistance: 0pR-1000=0.01%+7mQ	itions ±4.0°C % ±10% ation Serial No tor 1089G08 na 200uA-2mA=0.05%+300nA uV 20mV-200mV=30ppm+6nu/ uV 20mV-200mV=0.4%+150uV sha 200uA-2mA=0.05%+300nA uV 20mV-200mV=0.0%+450uV na 200uA-2mA=0.05%+300nA uV 20mV-20mV-30ppm+6nu/ uV 20mV-20mV-30ppm+6nu/ ivV 20mV-30ppm+6nu/ ivV 20mV-30pm-6nu/ ivV 20mV-30ppm-6nu/ ivV 20mV-3	Cert No	Cal Date 08 May 2009 100mA-2A=0.1%+0.5mA 2A-20A=0.2%+5m 10V-20V=0.3%+3mV (45Hz-10kHz) 20V-4 10V=0.9%+3mV (45Hz-10kHz) 20V-4 10V=0.0%+10Ω 1MΩ-10MΩ=0.02%+100mf 19 May 2009 100mA-2A=0.1%+0.5mA 2A-20A=0.2%+5m 1) 2V-20V=0.3%+3mV (45Hz-10kHz) 20V-2 10V=0.03%+3mV (45Hz-10kHz) 20V-2 10V=0.04%+10Ω 1MΩ-10MΩ-0.02%+100mf	Cal Due 07 May 2010 IA 100V=0.06%+20mV 200V- 0ppm+2mA 0mV 1 10MΩ-120MΩ=0.1%+1kΩ 18 May 2010 IA 100V=0.06%+20mV 200V- 0ppm+2mA 0mV





CERTIFICATE OF CALIBRATION

Issued By: Time Electronics

Date of Issue: 20 May 2009

Certificate Number DM10005

Page 2 of 3

Test Name	Rqd Value	Actual Value	Allowed Error	% of Spec	Pass/Fai
UPPER DISPLAY					
Voltage Measure					
0V DC	0.000V	0.000V	±0.002V	0%	Pass
15V DC	15.000V	14.997V	±0.005V	-60%	Pass
20V DC	20.000V	19.997V	±0.006V	-50%	Pass
30V DC	30.000V	29.997V	±0.008V	-38%	Pass
mA Measure					
4mA	4.000mA	4.000mA	±0.003mA	0%	Pass
12mA	12.000mA	11.999mA	±0.005mA	-20%	Pass
24mA	24.000mA	23.994mA	±0.007mA	-86%	Pass
LOWER DISPLAY					
mV/TC Measure					
0mV DC	0.00mV	0.01mV	±0.02mV	50%	Pass
45mV DC	45.00mV	45.00mV	±0.03mV	0%	Pass
90mV DC	90.00mV	89.99mV	±0.04mV	-25%	Pass
Voltage Measure					
0V DC	0.000V	0.000V	±0.002V	0%	Pass
10V DC	10.000V	9.999V	±0.004V	-25%	Pass
20V DC	20.000V	19.998V	±0.006V	-33%	Pass
Freqency Measure					
10kHz	10.00kHz	10.00kHz	±0.02kHz	0%	Pass
mA Measure					
4mA	4.000mA	4.000mA	±0.003mA	0%	Pass
12mA	12.000mA	12.000mA	±0.005mA	0%	Pass
24mA	24.000mA	23.997mA	±0.007mA	-43%	Pass
Thermocouple Meas	sure				
CJC Value	25.00°C	23.40°C	±5°C	-32%	Pass
0°C	0.00°C	-0.20°C	±0.7°C	-29%	Pass
Resistance 4 Wire N	leasure				
15Ω	15.00Ω	15.00Ω	±0.1Ω	0%	Pass
350Ω	350.00Ω	349.90Ω	±0.1Ω	-100%	Marginal
500Ω	500.0Ω	500.0Ω	±0.5Ω	0%	Pass
1500Ω	1500.0Ω	1499.8Ω	±0.5Ω	-40%	Pass
3200Ω	3200.0Ω	3198.7Ω	±1Ω	-130%	Fail
Resistance/RTD 3 W	/ire Measure				
350Ω	350.00Ω	350.02Ω	±0.1Ω	20%	Pass

Cert.rpt v8.1

This certificate has been produced by EasyCal Calibration Software from Time Electronics Ltd

CERTIFICATE OF CALIBRATION

Certificate Number DM10005

Issued By: Time Electronics

Date of Issue: 20 May 2009

Page 3 of 3

Test Name	Rqd Value	Actual Value	Allowed Error	% of Spec	Pass/Fail
Voltage Source					
0V	0.0000V	0.0000V	±0.002V	1%	Pass
5V	5.0000V	5.0001V	±0.003V	5%	Pass
10V	10.0000V	10.0005V	±0.004V	12%	Pass
mV Source					
0mV	0.000mV	0.002mV	±0.02mV	10%	Pass
45mV	45.000mV	44.996mV	±0.03mV	-14%	Pass
100mV	100.000mV	99.997mV	±0.04mV	-8%	Pass
Frequency Source					
10kHz	10.0000kHz	10.0000kHz	±0.025kHz	0%	Pass
mA Source					
4mA	4.0000mA	4.0004mA	±0.0028mA	13%	Pass
12mA	12.0000mA	11.9996mA	±0.0044mA	-9%	Pass
24mA	24.0000mA	23.9989mA	±0.0068mA	-16%	Pass
Ohms Source					
15Ω	15.0Ω	15.0Ω	±0.1Ω	15%	Pass
360Ω	360.0Ω	360.0Ω	±0.1Ω	23%	Pass
500Ω	500.0Ω	500.2Ω	±0.5Ω	30%	Pass
Thermocouple Source					
Cold Junction Value	-25.00°C	-23.83°C	±5°C	-23%	Pass
0°C	0.00°C	0.12°C	±0.7°C	17%	Pass
180°C	180.00°C	180.19°C	±0.7°C	28%	Pass
-180°C	-180.00°C	-179.46°C	±0.7°C	-77%	Pass

Comments

Cert.rpt v8.

 ${\it This certificate has been produced by EasyCal\ Calibration\ Software\ from\ Time\ Electronics\ Ltd}$





CALIBRATION REPORT

Page 1 of 1

Issued By: Laboratory

Certificate Number: 10060

Device Information

Device TAG / ID: TMP_TX Type: Temperature Transmitter Model: Example 0-150°C 4-20mA Serial Number: 09091789 Location:AREA 996

Procedure Information

Procedure:TMP-TX Input Range:0.00 to 150.00°C Output Range:4.00 to 20.00mA Reject Error >:0.50% of Range

Calibration Information

Calibration Date : 08 May 2011 Due Date: 06 May 2012 (52wks) Temperature: 22.0°C Relative Humidity: 50%

Comments:


 Calibrator Information

 Description
 Serial No.
 Cert No.
 Cal Date
 Cal Due

 5051+ (DMM mode)
 1039C11
 0313989
 12 Apr 2011
 10 Apr 2012

 Temperature Standard
 Example
 Example
 12 Apr 2011
 09 Apr 2013

Test Point	Input Temperature	Nominal Output	Actual	Allowed Error	% of Range	
			Output			Pass/Fail
0%	0.00°C	4.00mA	4.03mA	±0.1mA	0.1725%	Pass
20%	30.00°C	7.20mA	7.22mA	±0.1mA	0.1035%	Pass
40%	60.00°C	10.40mA	10.44mA	±0.1mA	0.1800%	Pass
60%	90.00°C	13.60mA	13.62mA	±0.1mA	0.1242%	Pass
80%	120.00°C	16.80mA	16.82mA	±0.1mA	0.1031%	Pass
100%	150.00°C	20.00mA	20.02mA	±0.1mA	0.1205%	Pass
End Of Results						

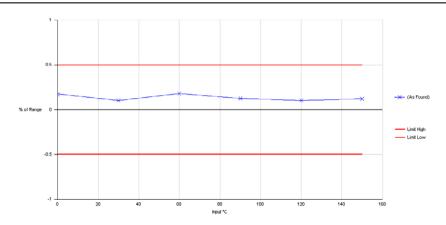

Comments:

Calibrated by: Op 1 Aprroved By:Sig 3 Signed:

Aprroved Date:16-May-2011

DeviceCert.rpt v1.5

This certificate has been produced by EasyCal Calibration Software from Time Electronics Ltd



Job No. EC2/131107

Ident: EC2

Status: WAITING INFO
Date Recieved: 13-Nov-07

Type: Multimeter

Model: 87

Ser No.: 12345

Service Rq'd: RE-CALIBRATION

MARTIN ANDREWS

Cal Systems Ltd

Returned with

Packing

Battery





ID: 2599 Serial: 77460532



DO NOT REMOVE

Laboratory

EasyCal

Cert No. : 10001 Serial No. : 52775/8V Cal Due : 10/June/2010

CALIBRATED 11/June/2009

I**D**: TF401

S/N: 52775/8V



DO NOT REMOVE

EasyCal Ordering Information

Licensing details, add-ons, and EasyCal accessory codes



Primary Licenses









Full CalStation and Work Station license with 1 year support.

Order Code: ECFL







EasyCal Full License (when purchased with compatible calibrator/DMM)

Discounted Full CalStation and Work Station license with 1 year support.

Order Code: ECFLA

Extra User License Options







EasyCal Additional Full License (secondary user)

Discounted Full Licence for additional users.

Order Code: EC2FL





Additional EasyCal Work Station License

Allows Job Management, Cal Due Instrument Attachments / Cert History, Batch Instrument Edit and Procedure Wizards. Suitable for users not requiring CalRun (ie front office).

Order Code: EC2WL

Add-Ons



x2

EasyAdmin - 2 Users

Security add-on that enables setting of user rights, access levels, and more.

For installations of 2 users or less. Order Code: EAD2



x5

EasyAdmin - 5 Users

Security add-on that enables setting of user rights, access levels, and more.

For installations of 5 users or less. Order Code: EAD5



x10

EasyAdmin - 10 Users

Security add-on that enables setting of user rights, access levels, and more.

For installations of 10 users or less. Order Code: EAD10



x10 +

EasyAdmin - 10+ Users

Security add-on that enables setting of user rights, access levels, and more.

For installations of over 10 users. Order Code: EAD10+





WebCerts

Online application enabling upload and retrieval of certificates and reports

Order Code: EWC







WebCerts - Hosted by Time Electronics

Online application enabling upload and retrieval of certificates and reports.

Order Code: EWCTE

Hardware Options, Additional Software and Support Packages

9777	Bar Code Reader
9778	Cal and ID Label Printer
9779	Job and Address Label Printer
9743	PCI to GPIB Interface card
9794	USB to GPIB Interface Adaptor
9597	GPIB Cable
9588	RS-232 Cable
9765	RS-232 to USB Interface Adaptor
CREP	Crystal Reports Sofware: Edit and format certificate styles
ESP1	EasyCal Support Package 1: 1 year email & telephone support. Minor Upgrades.
ESP2	EasyCal Support Package 2: 2 year email & telephone support. Minor Upgrades.
EOT1	EasyCal Online Training (Via Remote Desktop).



Time Electronics Ltd., Unit 11 Sovereign Way,
Botany Industrial Estate, Tonbridge, Kent, TN9 1RH. United Kingdom.
T: +44 (0) 1732 355993 F: +44 (0) 1732 770312 E: mail@timeelectronics.co.uk

www.timeelectronics.com

For more information please contact your local Time Electronics representative: